

mectron

WE ♥ PRO
PHYLAXIS

WE ♥ PRO
PHYLAXIS

WE ♥ PRO
PHYLAXIS

→ MECTRON
ULTRASONIC INSERTS




→ ULTRASONIC INSERTS

→ MULTIPIEZO

→ A LARGE VARIETY OF APPLICATIONS

Scaling, perio, endo, restorative – Mectron offers a wide range of applications. Mectron's high-quality technique guarantees optimal treatment power and utmost security in each single unit.

This remarkable quality is the result of the successful combination of fine electronic concept and a special tips design.

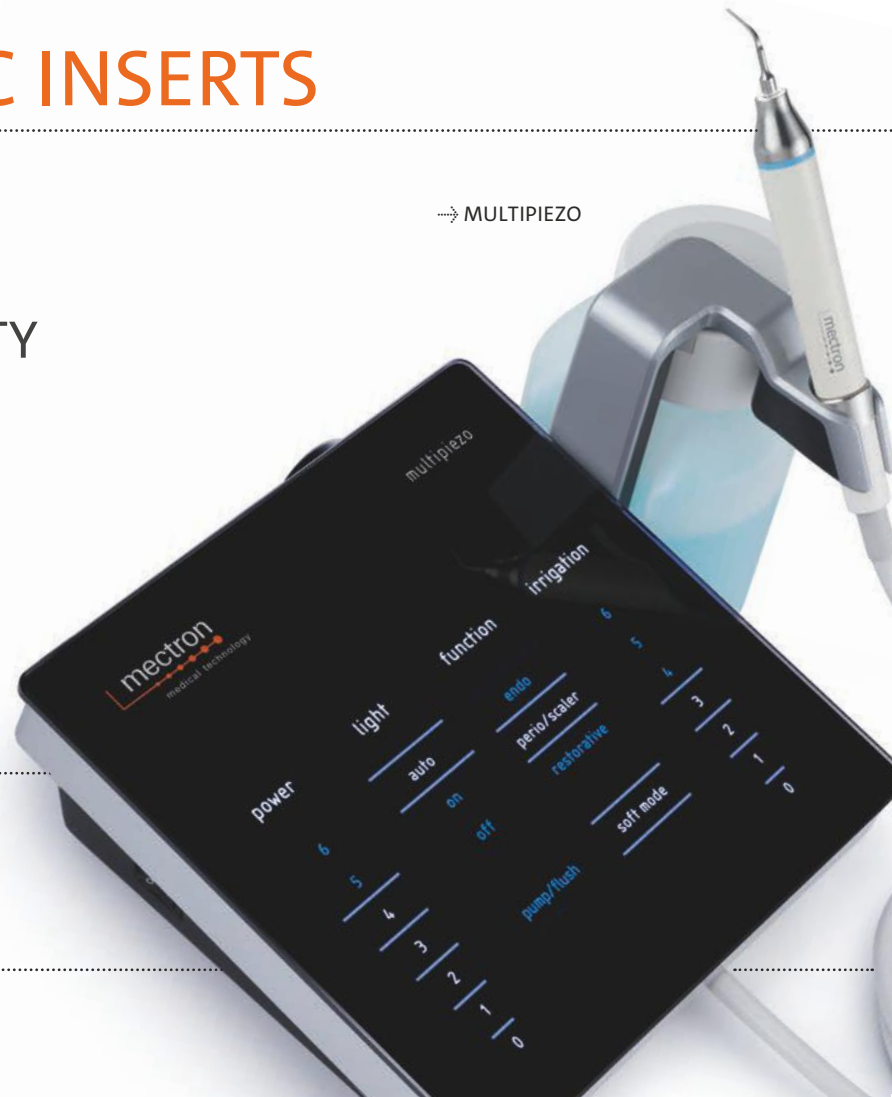

→ COMBI touch



→ MICROPIEZO



→ COMPACT PIEZO LED



→ COMPACT PIEZO P2K



→ THE INSERTS




Mectron offers an unequalled variety of inserts – for every indication, every treatment, and every situation you will face in your daily practice. More than 30 different inserts are available.

→ TORQUE WRENCH K10



→ TORQUE WRENCH K10 – PROTECTS YOUR HANDPIECE AND INSERTS

- sterilisable
- inserts are supplied with their own dynamometric wrench

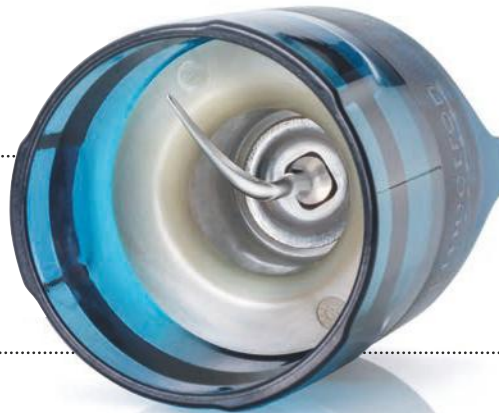

CONTENTS

→ 8-14 INSERT SETS

- 8/9 Set maintenance/Set scaling
- 10/11 Set perio maintenance/Set perio treatment
- 12/13 Set implant cleaning/Set ortho clean-up
- 14 Set endo revision

→ 16-22 SCALING INSERTS

- 16/17 Insert S1/Insert S1-S
- 18/19 Insert S2/Insert S3
- 20/21 Insert S4/Insert S5
- 22 Insert S6

→ 24-27 PERIO UNIVERSAL INSERTS

- 24/25 Insert P1/Insert P2
- 26/27 Insert P3/Insert P4

→ 28-35 PERIO ANATOMIC INSERTS

- 28/29 Insert P10/Insert P11
- 30/31 Insert P12/Insert P13
- 32/33 Insert P14/Insert P15
- 34/35 Insert P16R/Insert P16L

→ 36-37 IMPLANT CLEANING INSERT

→ 38-39 ORTHODONTIC CLEAN-UP INSERTS

- 38/39 Insert D05120/Insert D07102 + tip D06007

→ 40-45 ENDO REVISION INSERTS

- 41 Insert ER1
- 42/43 Insert ER2/Insert ER3
- 44/45 Insert ER4/Insert ER5

→ 46-49 ENDO RETRO INSERTS

- 47 Insert RD3
- 48/49 Insert RD4/Insert RD5

→ 50-53 EXTRACTION INSERTS

- 51 Insert ME1
- 52/53 Insert ME2/Insert ME3

→ 54-55 CROWN PREP TIPS

→ 56-59 APPROPRIATE INSERT SETTINGS

→ 60-61 REFERENCE NUMBERS/TIP CARD

→ SET MAINTENANCE

→ EQUIPPED WITH:

- 1 insert S1
- 1 insert S2
- 1 insert S5
- 1 insert P2
- 1 insert P3
- 5 torque wrenches K10



→ SET SCALING

→ EQUIPPED WITH:

- 1 insert S1
- 1 insert S2
- 1 insert S3
- 1 insert S4
- 1 insert S5
- 5 torque wrenches K10



→ SET PERIO MAINTENANCE

→ EQUIPPED WITH:

- 1 insert P10
- 1 insert P11
- 1 insert P12
- 1 insert P13
- 1 insert P14
- 5 torque wrenches K10



→ SET PERIO TREATMENT



→ EQUIPPED WITH:

- 1 insert P2
- 1 insert P3
- 1 insert P15
- 1 insert P16R
- 1 insert P16L
- 5 torque wrenches K10



→ SET IMPLANT CLEANING

→ EQUIPPED WITH:

- 1 insert ICS
- 1 torque wrench K10
- 5 Implant cleaning tips IC1



→ ICS




→ IC1

→ SET ORTHO CLEAN-UP*

→ EQUIPPED WITH:

- 1 insert D05120
- 1 insert D07102
- 2 torque wrenches K10
- 5 D06007 tips

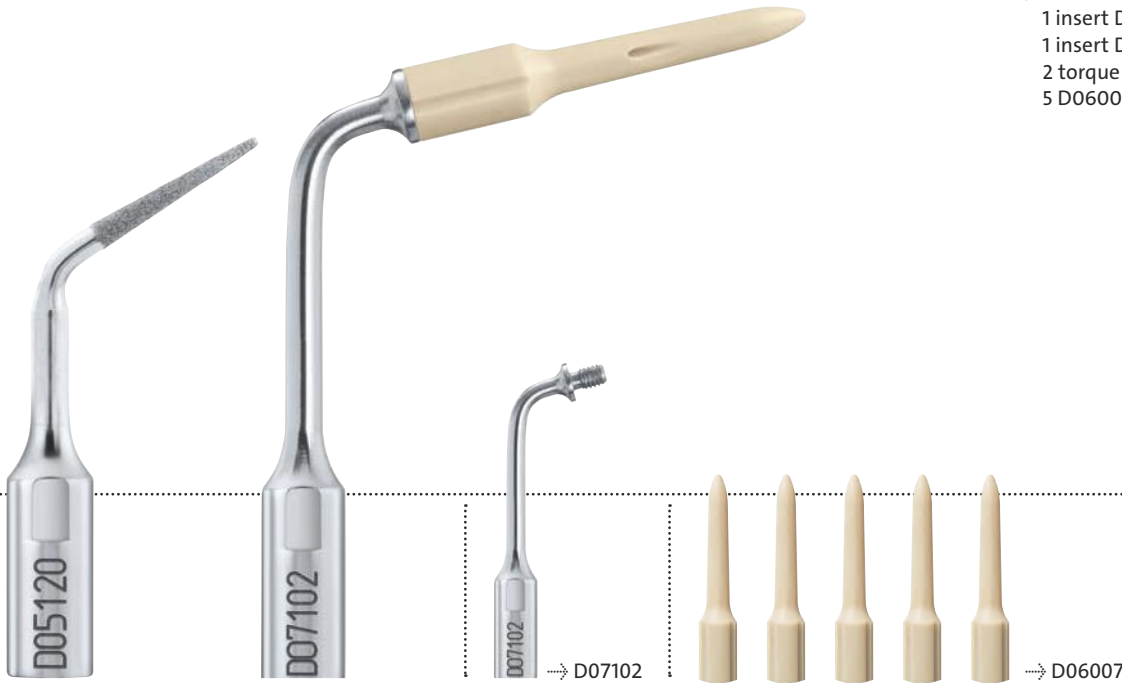

INSERT SETS


→ SET ENDO REVISION

→ EQUIPPED WITH:

- 1 insert ER1
- 1 insert ER2
- 1 insert ER3
- 1 insert ER4
- 1 insert ER5
- 5 torque wrenches K10





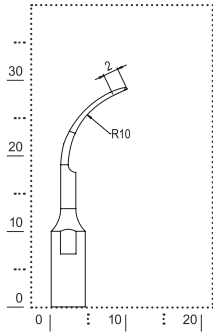

→ IDENTIFICATION

scaling

→ MORPHOLOGY


universal curette with semicircular diameter

→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for considerable tartar removal





→ IDENTIFICATION

perio/scaling

→ MORPHOLOGY



long universal curette with triangled
slightly curved surface


→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for supragingival tartar removal
and subgingival concretions and
biofilm elimination

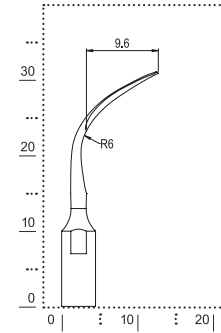

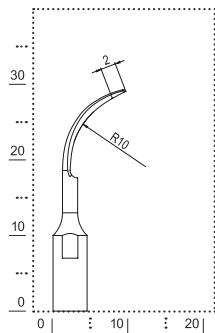


→ IDENTIFICATION
scaling

→ MORPHOLOGY
universal curette with triangled,
slightly curved surface

→ SURFACE
brightly polished medical grade stainless steel

→ TREATMENT
efficient in the interdental spaces
and posterior surfaces





→ **IDENTIFICATION**

scaling

→ **MORPHOLOGY**


flat, with rounded edges


→ **SURFACE**

brightly polished medical grade stainless steel

→ **TREATMENT**

for considerable supragingival
tartar removal

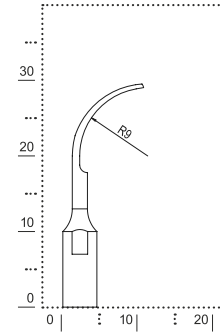

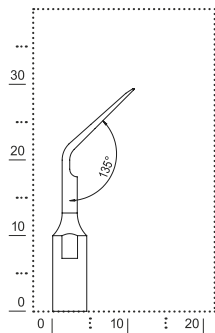

→ IDENTIFICATION

scaling

→ MORPHOLOGY

universal curette with 45° angled, triangled and slightly curved surface

→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for tartar removal on mesial and distal interdental surfaces in the posterior area





→ IDENTIFICATION

scaling

→ MORPHOLOGY



similar shape to S1 insert
but longer and thinner


→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for gentle supra- and subgingival
tartar removal and for gingivitis

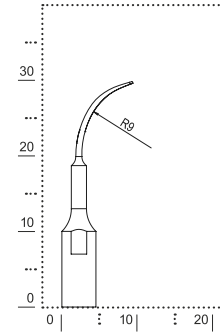

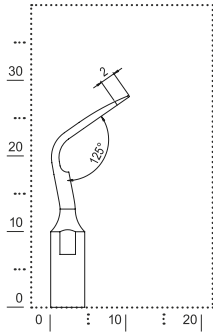

→ IDENTIFICATION

scaling

→ MORPHOLOGY


contra-angled universal curette with
semicircular diameter


→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

powerful insert (twice the power of S1 insert)
for considerable tartar removal



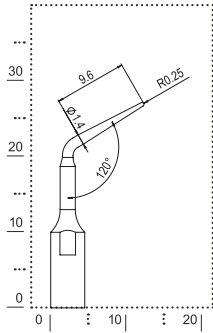

→ IDENTIFICATION

perio

→ MORPHOLOGY

long, straight working tip with a circular surface

→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for concrements and biofilm
removal from root surfaces





→ IDENTIFICATION

perio

→ MORPHOLOGY



curved working tip with a circular surface


→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for concrements and biofilm
removal from root surfaces

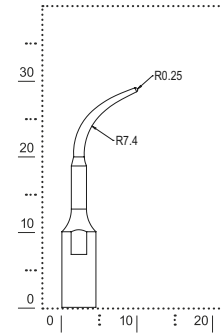

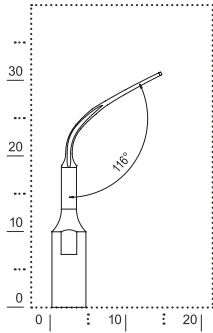

→ IDENTIFICATION

perio

→ MORPHOLOGY



slim and smooth like a probe

→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

supra and subgingival concretions and
biofilm removal from interproximal spaces





→ IDENTIFICATION

perio

→ MORPHOLOGY


extra long, straight working tip
with a circular surface


→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for concrements and biofilm removal
from root surfaces

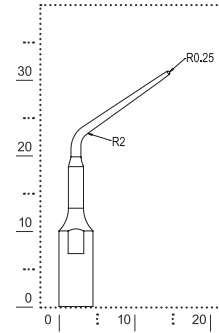

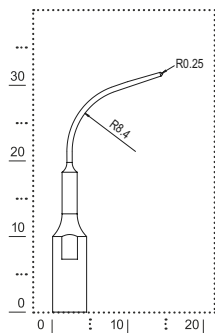

→ IDENTIFICATION
perio

→ MORPHOLOGY
extra long, curved working tip
with a circular surface

→ SURFACE
brightly polished medical grade stainless steel

→ TREATMENT
for concrements and biofilm removal
from root surfaces





→ IDENTIFICATION

perio

→ MORPHOLOGY


right (inclination of 15°) curved insert
with round tip


→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for gentle subgingival concretions removal

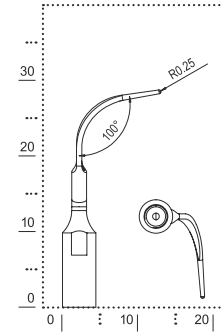

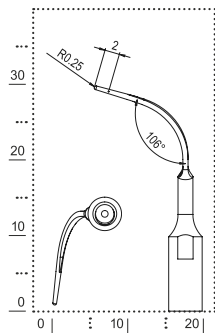

→ IDENTIFICATION

perio

→ MORPHOLOGY

left (inclination of 15°) curved insert
with round tip

→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for gentle subgingival concretions removal





→ IDENTIFICATION

perio

→ MORPHOLOGY


right (inclination of 15°) curved insert
with spherical ($\varnothing = 0.8 \text{ mm}$) round tip


→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for concrements and biofilm removal
in furcations and concavities

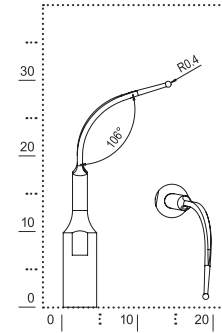

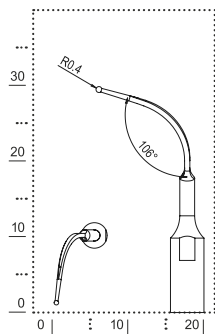

→ IDENTIFICATION

perio

→ MORPHOLOGY

left (inclination of 15°) curved insert
with spherical ($\varnothing = 0.8$ mm) round tip

→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

for concrements and biofilm removal
in furcations and concavities





→ IDENTIFICATION

perio

→ MORPHOLOGY



universal curette shape with round surface

→ SURFACE


brightly polished medical grade stainless steel

→ TREATMENT

supra- and subgingival concretions and biofilm removal. Recommended for the treatment of canine and anterior teeth. Debridement of deep periodontal pockets.

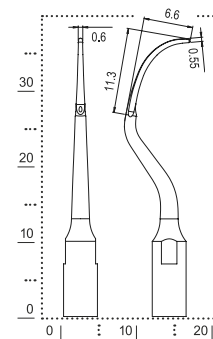

P16R

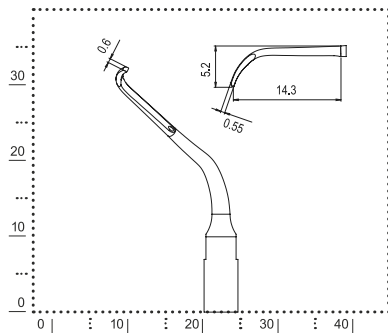

→ IDENTIFICATION

perio

→ MORPHOLOGY


right angled periodontal curette

→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT

subgingival concretions and biofilm removal from furcations and deep pockets. Recommended for the treatment of molars and premolars.

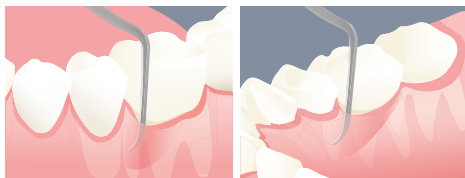



→ IDENTIFICATION

perio

→ MORPHOLOGY



left angled periodontal curette

→ SURFACE

brightly polished medical grade stainless steel

→ TREATMENT


subgingival concretions and biofilm removal from furcations and deep pockets. Recommended for the treatment of molars and premolars.

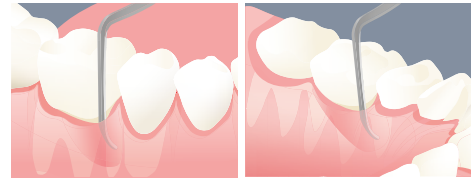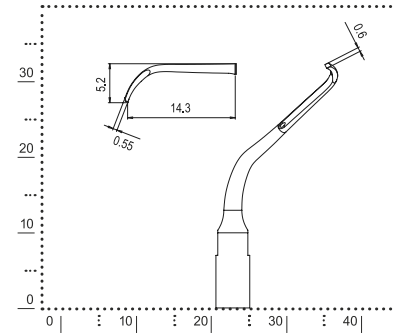

→ ICS + IC1

→ INSERT FOR IMPLANT CLEANING – MAXIMAL TREATMENT EFFICIENCY WITH THE HIGHEST PATIENT COMFORT

- tip IC1 – 100% PEEK (high tech plastics) – for the maximum respect of the implant surface
- the special shape of the tipholder ICS allows an optimal access and a perfect view even in posterior regions
- tipholder ICS and tip IC1 are both sterilisable and reusable

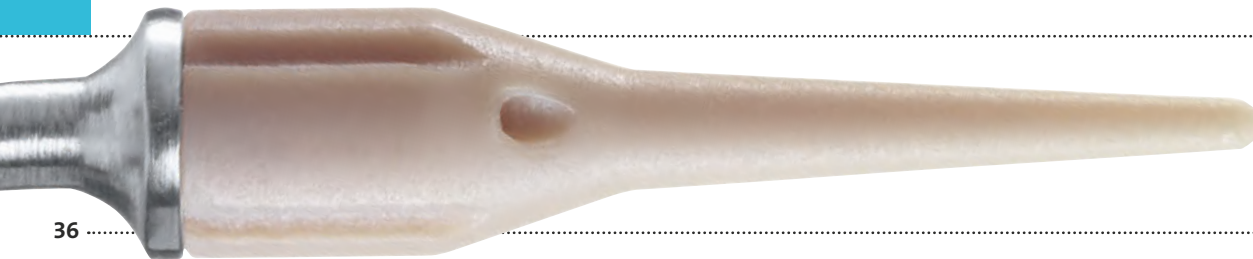

→ IMPLANT CLEANING SET S

The set consists
of a tipholder ICS,
1 torque wrench K10
and 5 tips IC1



→ IDENTIFICATION

perio

→ MORPHOLOGY



102° angled tipholder with conical PEEK tip
(working length 10 mm, $\varnothing$ top 0.8 mm,
 $\varnothing$ base 2 mm)

→ SURFACE

brightly polished medical grade stainless steel
for tipholder ICS and 100% PEEK for IC1

→ TREATMENT

efficient and gentle cleaning of implants
and restorations

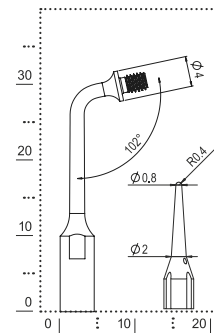


→ ICS



→ IC1

implant cleaning tip IC1
can be easily tightened
without special tools
and is fully autoclavable

→ D05120

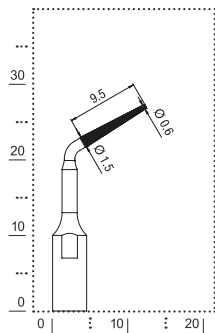

→ IDENTIFICATION

restorative

→ MORPHOLOGY

angled insert with $\text{Ø } 0.60 > \text{Ø } 1.50$, working length 9.5 mm, D30 diamond coated

→ SURFACE

brightly polished medical grade stainless steel D30 diamond coated

→ TREATMENT

safe and effective removal of the residual adhesive post orthodontic therapy (fixed, removable/invisible)





D07102 + D06007



→ IDENTIFICATION

restorative

→ MORPHOLOGY


102° angled tipholder with conical PEEK tip
(working length 11.5 mm, Ø top 0.92 mm,
Ø base 2.4 mm)

→ SURFACE

brightly polished medical grade stainless steel for
tipholder D07102 and PEEK for tip D06007

→ TREATMENT

gentle polishing post removal of residual adhesive

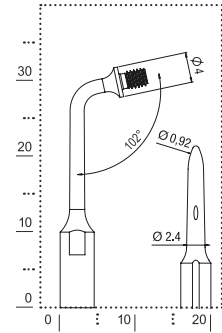

→ D07102



→ D06007

The tip D06007 made of PEEK is gentle on the enamel surface

→ ENDO REVISION WITH ER INSERTS

Exposure and removal of root pins, fast and effective removal of calcification in the coronal third of the root, removal of fractured root inserts – the ER inserts cover the complete spectrum of endodontic revision treatment.





→ IDENTIFICATION

endo revision

→ MORPHOLOGY


angled shaft with small, spherical ($\varnothing 1.7 \text{ mm}$)
and D30 diamond coated tip


→ SURFACE

titanium nitride coat

→ TREATMENT

exposure of root canal pins

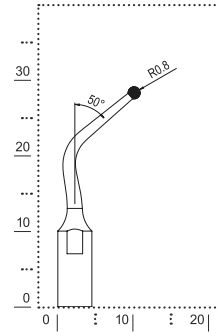

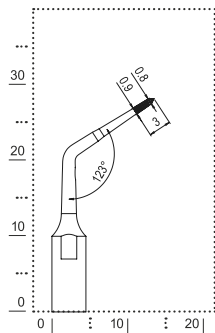

→ IDENTIFICATION

endo revision

→ MORPHOLOGY

angled insert with 0.7 mm Ø, working length up to 10 mm, the last 5 mm D30 diamond coated

→ SURFACE

titanium nitride coat

→ TREATMENT

location of concealed or calcified root canal entrances, removal of restoration materials, calcification and fractured inserts in the coronal third of the root canal





→ IDENTIFICATION

endo revision

→ MORPHOLOGY


angled insert with 0.6 mm Ø, working length up to 10 mm, the last 5 mm D30 diamond coated

→ SURFACE


titanium nitride coat

→ TREATMENT

presentation of calcified root canals entrances, removal of root elements and fractured inserts in the coronal third of the root canal

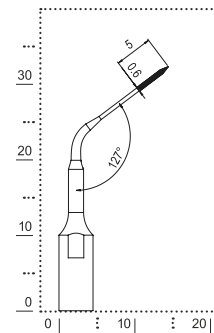

ER4

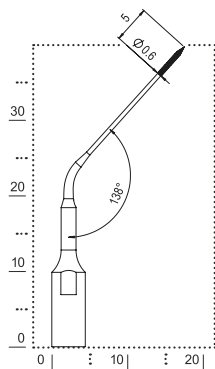

→ IDENTIFICATION

endo revision

→ MORPHOLOGY

angled insert with 0.6 mm Ø, working length up to 20 mm, the last 5 mm D30 diamond coated


→ SURFACE

titanium nitride coat

→ TREATMENT

presentation of calcified root canals entrances, removal of root elements and fractured inserts in the coronal third of the root canal



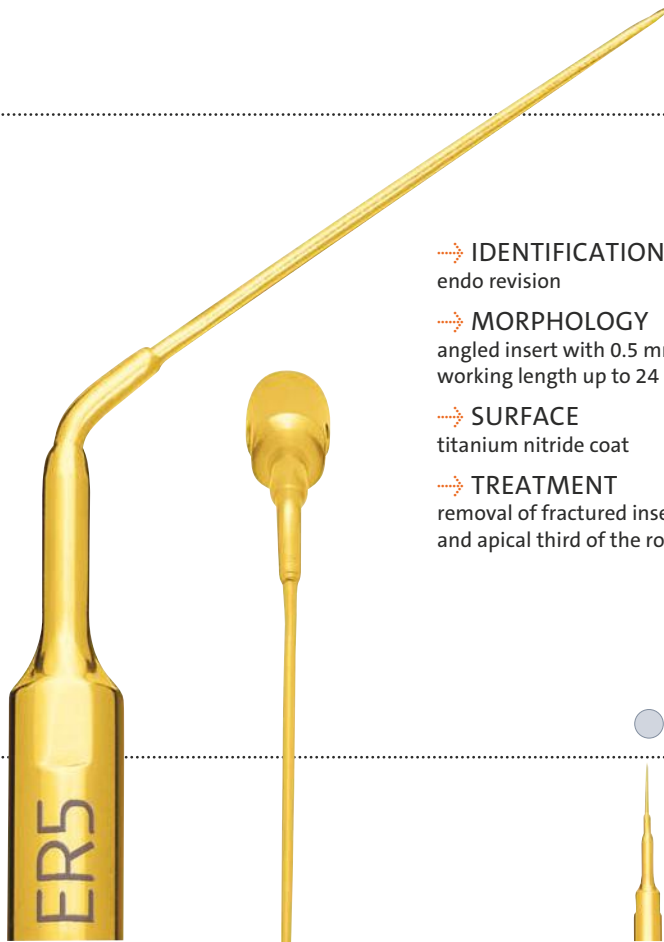

→ **IDENTIFICATION**

endo revision

→ **MORPHOLOGY**


angled insert with 0.5 mm $\varnothing$,
working length up to 24 mm

→ **SURFACE**

titanium nitride coat

→ **TREATMENT**


removal of fractured inserts in the medial
and apical third of the root canal

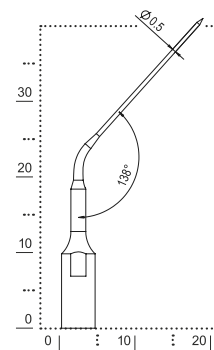


→ ENDO RETRO INSERTS – MINIMALLY INVASIVE RETROGRADE ROOT CANAL PREPARATION

Endo retro inserts assure a satisfying solution to the root canal access issue. Their thin and 90° angled structure allows a conservative cut through a minimum wide bone window.

These advantages facilitate wound healing and spare the patient useless pain.

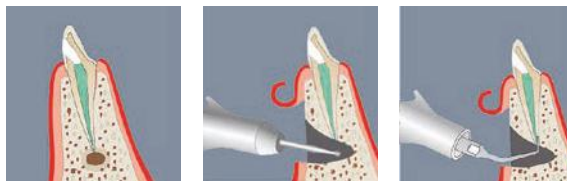

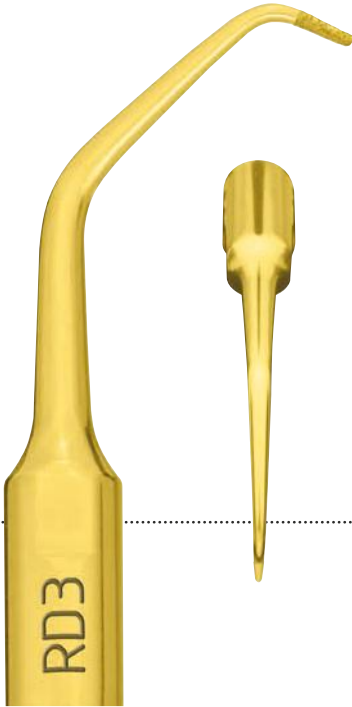

→ IDENTIFICATION

endo retro

→ MORPHOLOGY


angled shaft, with 90° angled working tip
and fine diamond coating (D30)


→ SURFACE

titanium nitride coat

→ TREATMENT

root canal cleaning in the frontal area

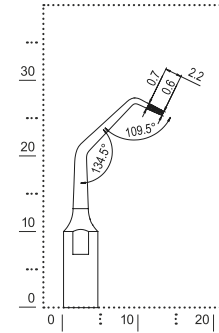

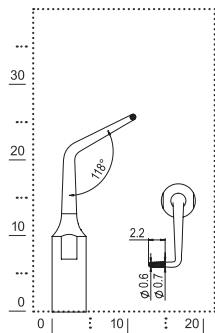

→ IDENTIFICATION

endo retro

→ MORPHOLOGY

angled shaft, with 90° right angled working tip and fine diamond coating (D30)


→ SURFACE

titanium nitride coat

→ TREATMENT

root canal cleaning in the molar area



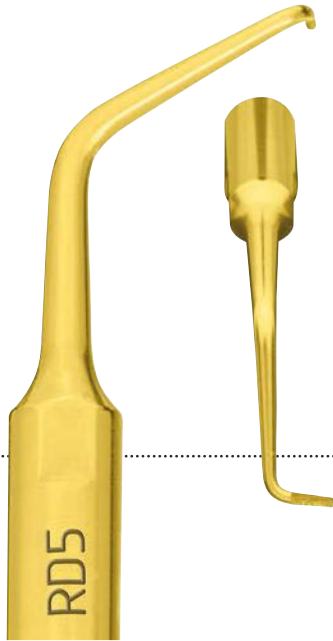

→ IDENTIFICATION

endo retro

→ MORPHOLOGY


angled shaft, with 90° left angled working tip
and fine diamond coating (D30)

→ SURFACE

titanium nitride coat

→ TREATMENT

root canal cleaning in the molar area

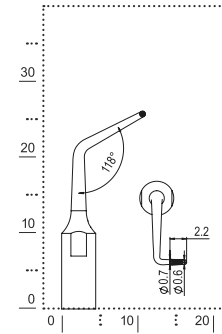

→ EXTRACTION INSERTS – EXCLUSIVE FOR UNITS WITH PULSE MODE

Even if the primary objective of dentistry is the preservation of natural teeth, sometimes extractions cannot be avoided. In these cases, maximum safety is the most important thing during treatment.

The specially shaped inserts ME1, ME2 and ME3 – with a blade thickness of only 0.35 mm – perfectly fulfill the anatomical demands of non surgical extractions. They offer maximum intra-operative sensitivity, allowing a great preservation of alveolar bone and periodontal tissues. Furthermore, the physiological solution guarantees maximum visibility thanks to the cavitation effect which leads to a temporary hemostasis of blood vessels.

→ EXCLUSIVE FOR UNITS WITH PULSE MODE

→ ME1*




→ IDENTIFICATION
extractions


→ MORPHOLOGY
double-edged blade with a thickness of only 0.35 mm

→ SURFACE
titanium nitride coat

→ TREATMENT
atraumatic teeth removal

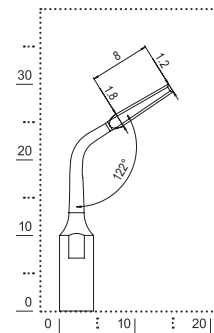

EXTRACTION INSERTS

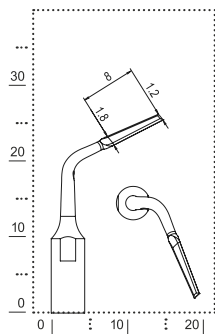

→ IDENTIFICATION

extractions

→ MORPHOLOGY


left angled, double-edged blade
with a thickness of only 0.35 mm

→ SURFACE

titanium nitride coat

→ TREATMENT

atraumatic teeth removal

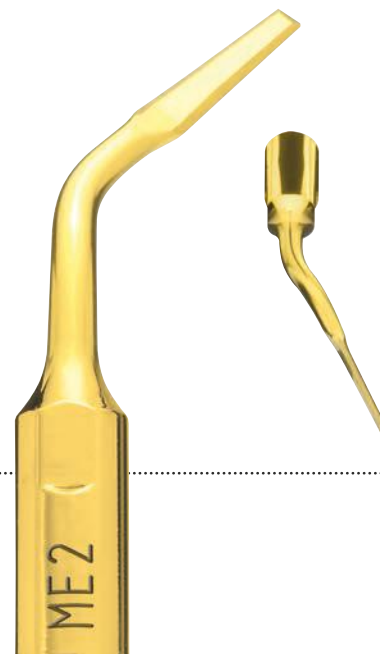


→ EXCLUSIVE FOR UNITS WITH PULSE MODE

→ ME3*



- IDENTIFICATION
extractions
- MORPHOLOGY
right angled, double-edged blade
with a thickness of only 0.35 mm
- SURFACE
titanium nitride coat
- TREATMENT
atraumatic teeth removal

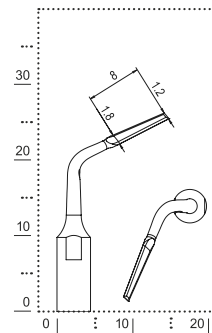

EXTRACTION INSERTS

CROWN PREP TIPS

CROWN PREP TIPS – ATRAUMATIC AND PRECISE

The crown prep tips are dedicated to the preparation and finishing of subgingival margins. Due to the particular morphology, the tip could be used in contact with the margin without damaging the surrounding soft tissues. The preparation margin could be positioned subgingivally giving more comfort to the patient.

The special shape of the tipholder allows an optimal view of the preparation field. The tipholder brings the crown prep tips to an elliptic movement and enables therefore a circular preparation of the tooth.


→ dynamometric wrench K7



→ key AB1



→ tip holder DB1 with crown prep tips

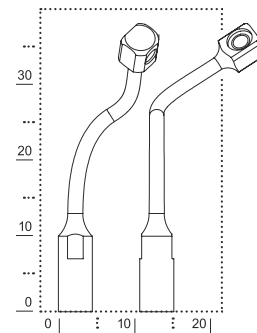

→ crown prep tip
TF12D60



→ VERTICAL PREPARATION TECHNIQUE

→ LENGTH 10 MM → DIAMOND COATING

diameter	D90	D60
1.2 mm	TF12D90	TF12D60
1.6 mm	TF16D90	TF16D60

→ CHAMFER TECHNIQUE

→ LENGTH 10 MM → DIAMOND COATING

diameter	D120	D90	D60
1.2 mm		TA12D90	TA12D60
1.4 mm	TA14D120	TA14D90	TA14D60
1.6 mm	TA16D120	TA16D90	TA16D60

→ crown prep tip
TA14D60



→ APPROPRIATE INSERT SETTINGS



function	endo	perio/scaler	restorative	endo	perio/scaler	restorative	endo	perio/scaler	prosthetics
----------	------	--------------	-------------	------	--------------	-------------	------	--------------	-------------

SCALING

S1-S		1-2**		1-2**		1-2**		1-2**	0-30%
S1, S2, S3, S4, S5, S6		1-6**		1-5**		1-3**			0-100%

PERIO

P1, P2, P3, P4, P10, P11, P12, P13, P14		1-3**		1-3**		1-3**			0-50%
P15, P16R, P16L		1-3**		1-3**		1-3**			0-50%

IMPLANT CLEANING

ICS + IC1		1-2**		1-2**		1-2**			0-30%
-----------	--	-------	--	-------	--	-------	--	--	-------

ORTHO CLEAN-UP

D05120, D07102 + D06007		3-6		3-5		3			50-100%
-------------------------	--	-----	--	-----	--	---	--	--	---------



function	endo	perio / scaler	restorative	endo	perio / scaler	restorative	endo	perio / scaler	prosthetics
----------	------	----------------	-------------	------	----------------	-------------	------	----------------	-------------

ENDO REVISION

ER1		1-6		1-5		1-3		0-100%	
ER2, ER3, ER4, ER5		1-3		1-3		1-3		0-50%	

ENDO RETRO

RD3, RD4, RD5		1-3		1-3		1-3		0-50%	
---------------	--	-----	--	-----	--	-----	--	-------	--

CROWN PREP

DB1		4-6		4-5		○**		50-100%	
-----	--	-----	--	-----	--	-----	--	---------	--

EXTRACTION


ME1, ME2, ME3 ***		6		5					
-------------------	--	---	--	---	--	--	--	--	--

* These devices are not provided with a power level indicator. The percentage value indicated in the table refers to the adjustment percentage of the scale of the potentiometer supplied with the device.

** Can be used with or without „soft mode“ function.

*** Not available in the United States and in Italy market.

→ APPROPRIATE INSERT SETTINGS

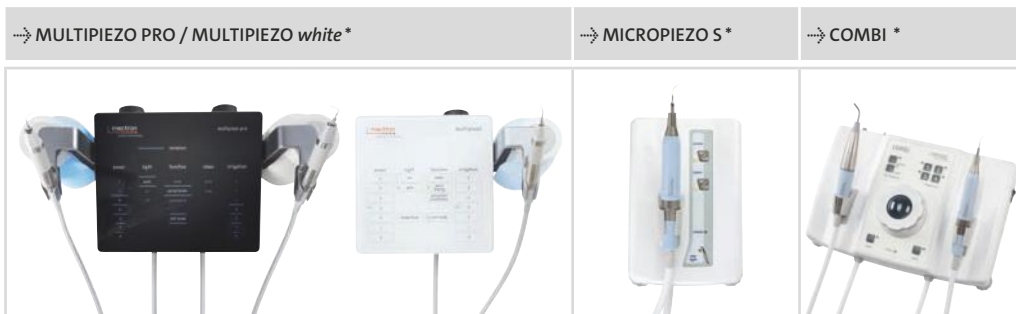

function	endo	perio / scaler	restorative / prosthetics	power	power
----------	------	----------------	---------------------------	-------	-------

SCALING

S1-S		1-2**		1-2	1-2
S1, S2, S3, S4, S5, S6		1-6**		1-6	1-4

PERIO

P1, P2, P3, P4, P10, P11, P12, P13, P14		1-3**		1-3	1-2
P15, P16R, P16L		1-3**		1-3	1-3

IMPLANT CLEANING

ICS + IC1		1-2**		1-2	1-2
-----------	--	-------	--	-----	-----

ORTHO CLEAN-UP

D05120, D07102 + D06007		3-6		3-6	2-4
-------------------------	--	-----	--	-----	-----

→ MULTIPIEZO PRO / MULTIPIEZO <i>white</i> *			→ MICROPIEZO S *	→ COMBI *
				
function	endo	perio / scaler	restorative / prosthetics	power

ENDO REVISION

ER1		1-6	3-6	2-4
ER2, ER3, ER4, ER5		1-3	1-3	1-2

ENDO RETRO

RD3, RD4, RD5		1-3	1-4	1-3
---------------	--	-----	-----	-----

CROWN PREP

DB1		4-6	4-6	3-4
-----	--	-----	-----	-----

EXTRACTION

ME1, ME2, ME3 ***		6		
-------------------	--	---	--	--



REFERENCE NUMBERS

→ ITEM/REFERENCE NUMBER	
set maintenance	02160035-001
set scaling	02160001-001
set perio maintenance	02160006-001
set perio treatment	02160036-001
set implant cleaning S*	02160033-001
set ortho clean-up **	02160037-001
set endo revision	02160008-001
torque wrench K10	02900137-001
dynamometric wrench K6	02900074
wrench K1	02270003
insert S1-S + wrench K10	02960009-001
insert S1 + wrench K10	02960001-001
insert S2 + wrench K10	02960002-001
insert S3 + wrench K10	02960003-001
insert S4 + wrench K10	02960004-001
insert S5 + wrench K10	02960005-001
insert S6 + wrench K10	02960006-001
insert P1 + wrench K10	02970001-001
insert P2 + wrench K10	02970002-001
insert P3 + wrench K10	02970003-001
insert P4 + wrench K10	02970004-001

→ ITEM/REFERENCE NUMBER	
insert P10 + wrench K10	03080001-001
insert P11 + wrench K10	03080002-001
insert P12 + wrench K10	03080003-001
insert P13 + wrench K10	03080004-001
insert P14 + wrench K10	03080005-001
insert P15 + wrench K10	03080006-001
insert P16R + wrench K10	03080007-001
insert P16L + wrench K10	03080008-001
tip holder ICS	03570004-001
tip IC1 (5 pieces)	02900112
insert D05120 + wrench K10	02990005-001
tipholder D07102 + wrench K10	02990007-001
tip D06007 (5 pieces)	02900190
insert ER1 + wrench K10	03450001-001
insert ER2 + wrench K10	03450002-001
insert ER3 + wrench K10	03450003-001
insert ER4 + wrench K10	03450004-001
insert ER5 + wrench K10	03450005-001
insert RD3 + wrench K10	03050006-001
insert RD4 + wrench K10	03050007-001
insert RD5 + wrench K10	03050008-001



→ ITEM/REFERENCE NUMBER	
insert ME1 + wrench K6	03130001-001
insert ME2 + wrench K6	03130002-001
insert ME3 + wrench K6	03130003-001
crown prep set***	02160009
tip holder DB1	03570001
key AB1	03580001
dynamometric wrench K7	02900081
crown prep tip TA12D60	03590001
crown prep tip TA14D60	03590002
crown prep tip TA16D60	03590003
crown prep tip TA12D90	03590004
crown prep tip TA14D90	03590005
crown prep tip TA16D90	03590006
crown prep tip TA14D120	03590007
crown prep tip TA16D120	03590008
crown prep tip TF12D60	03590010
crown prep tip TF16D60	03590011
crown prep tip TF12D90	03590012
crown prep tip TF16D90	03590013

* equipped with: ICS and 5 x IC1 + K10

** equipped with: D05120, D07102, 5 X D06007 + 2 K10

*** equipped with: AB1, DB1 + K7

MECTRON TIP CARD

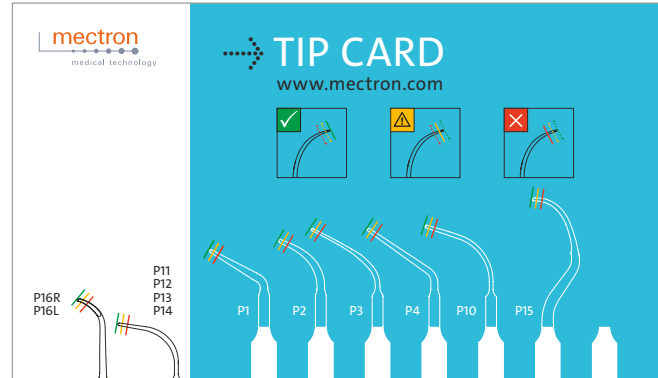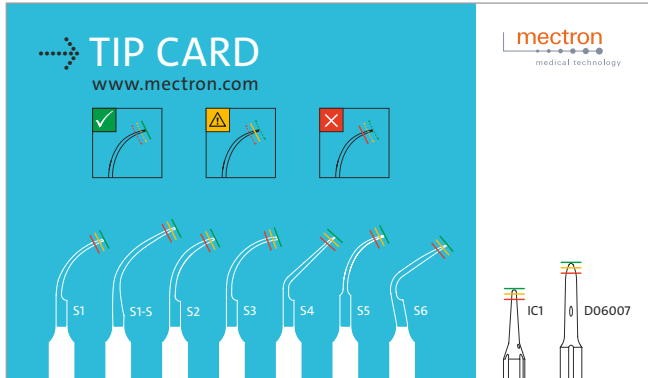

Ultrasonic inserts wear out the same as manual instruments. Regularly check your inserts by means of the erosion tip card. Whenever your inserts are shorter than the red hatched line, their performance is 50% less than the initial one. Such inserts should be quickly replaced.

NOTES

mectron s.p.a., via Loreto 15/A,
16042 Carasco (Ge), Italy,
tel +39 0185 35361, fax +39 0185 351374

→ www.mectron.com – mectron@mectron.com



© Copyright mectron S.p.A., Carasco, Italy
All rights reserved. Text, images and graphics contained in Mectron brochures are protected by copyright and other property rights laws. Content cannot be copied, disclosed, modified or made accessible to third parties for commercial purposes without written permission from Mectron S.p.A.

The images shown are for illustration purposes only and may not be an exact representation of the product. Please consult product labels and manual for indications, contraindications, hazards, warnings, cautions. Please contact your local sales representative for product availability.

All products illustrated in this brochure are CE-marked and registered in accordance with the EU Medical Device Regulation (MDR 2017/745). These medical devices are intended exclusively for use by qualified healthcare professionals. The content of this brochure is intended for healthcare professionals for informational and educational purposes only and does not constitute medical advice. Please refer to the Instructions for Use (IFU) and local regulations prior to use.

For graphic reasons the styling of the product names might be different. The registered product names correspond as following:

• combi touch	COMBI <i>touch</i>	• COMPACT PIEZO LED	COMPACT PIEZO LED
• multipiezo	MULTIPIEZO	• COMPACT PIEZO P2K	COMPACT PIEZO P2K
• MICROPIEZO	MICROPIEZO		